



File ..\DATA\2020\20201029\1140\BIZ2020-O28-SCH9.D Tgt Mass (CHM):
 Injection Date : 29 Oct 20 6:43 pm +0800 Seq. Line : 117
 Sample Name : BIZ2020-O28-SCH9 Location : P1-C-01
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 5 ul
 Acq. Method : D:\Chem32\1\data\2020\20201029\1140\1-POS-3MIN-1(500-2000).M
 Analysis Method : D:\CHEM32\1\DATA\2020\20201029\1140\1-POS-3MIN-1(500-2000).M
 Catalog No : HY-P1329A
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
 Oven Temperature : 45C
 Postive,MS:500-2000


DAD1 B, Sig=214,4 Ref=off

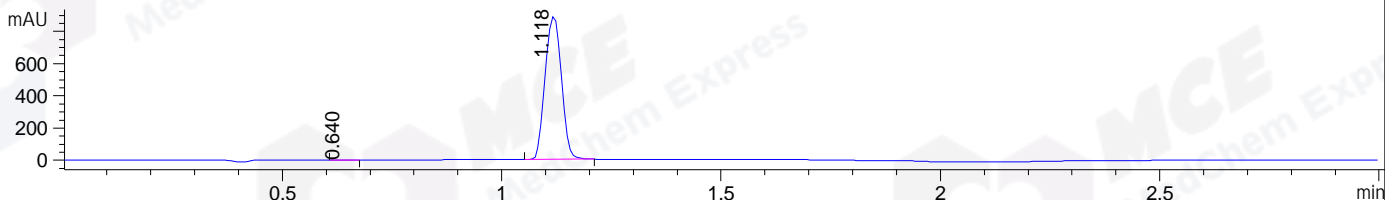


DAD1 C, Sig=254,4 Ref=off

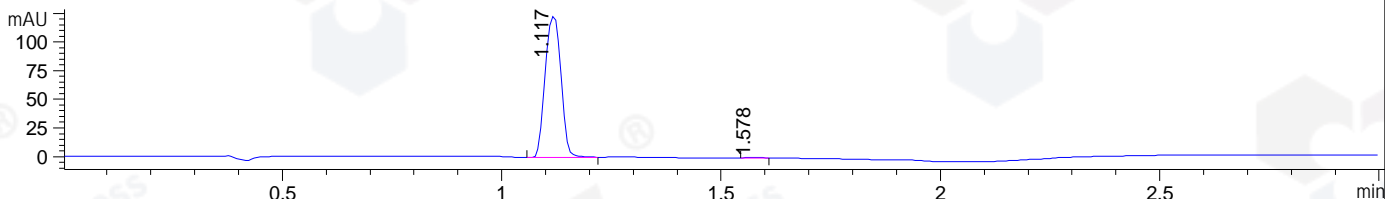

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

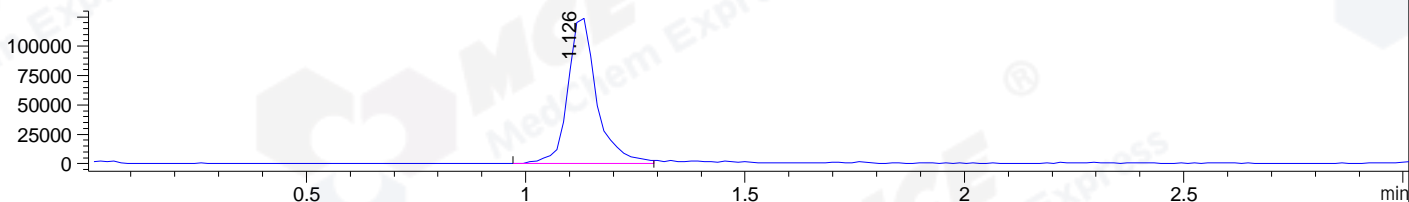

Ion 1177, MSD1 1177, Target Mass 1176 +H Positive, EIC=1176.7:1177.7

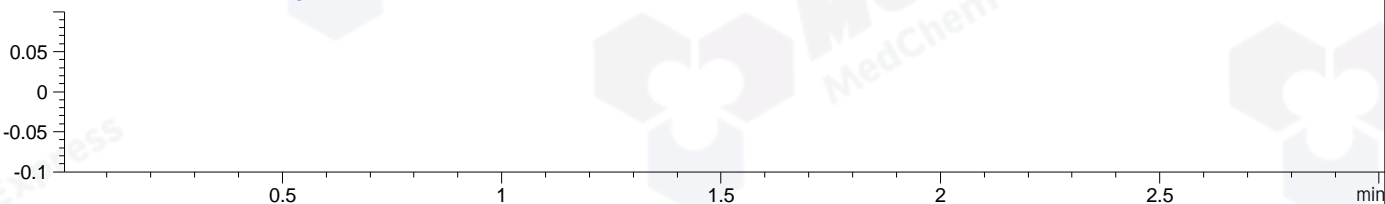

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.64	0.03	1.54	0.75	0.07	ND
1.12	0.04	2306.36	893.65	99.93	532

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.04	311.09	123.97	99.64	532
1.58	0.04	1.13	0.45	0.36	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.07	566213.81	126717.98	100.00	532

Ret. Time: 1.13

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

