


# MASS SPECTROMETRY REPORT

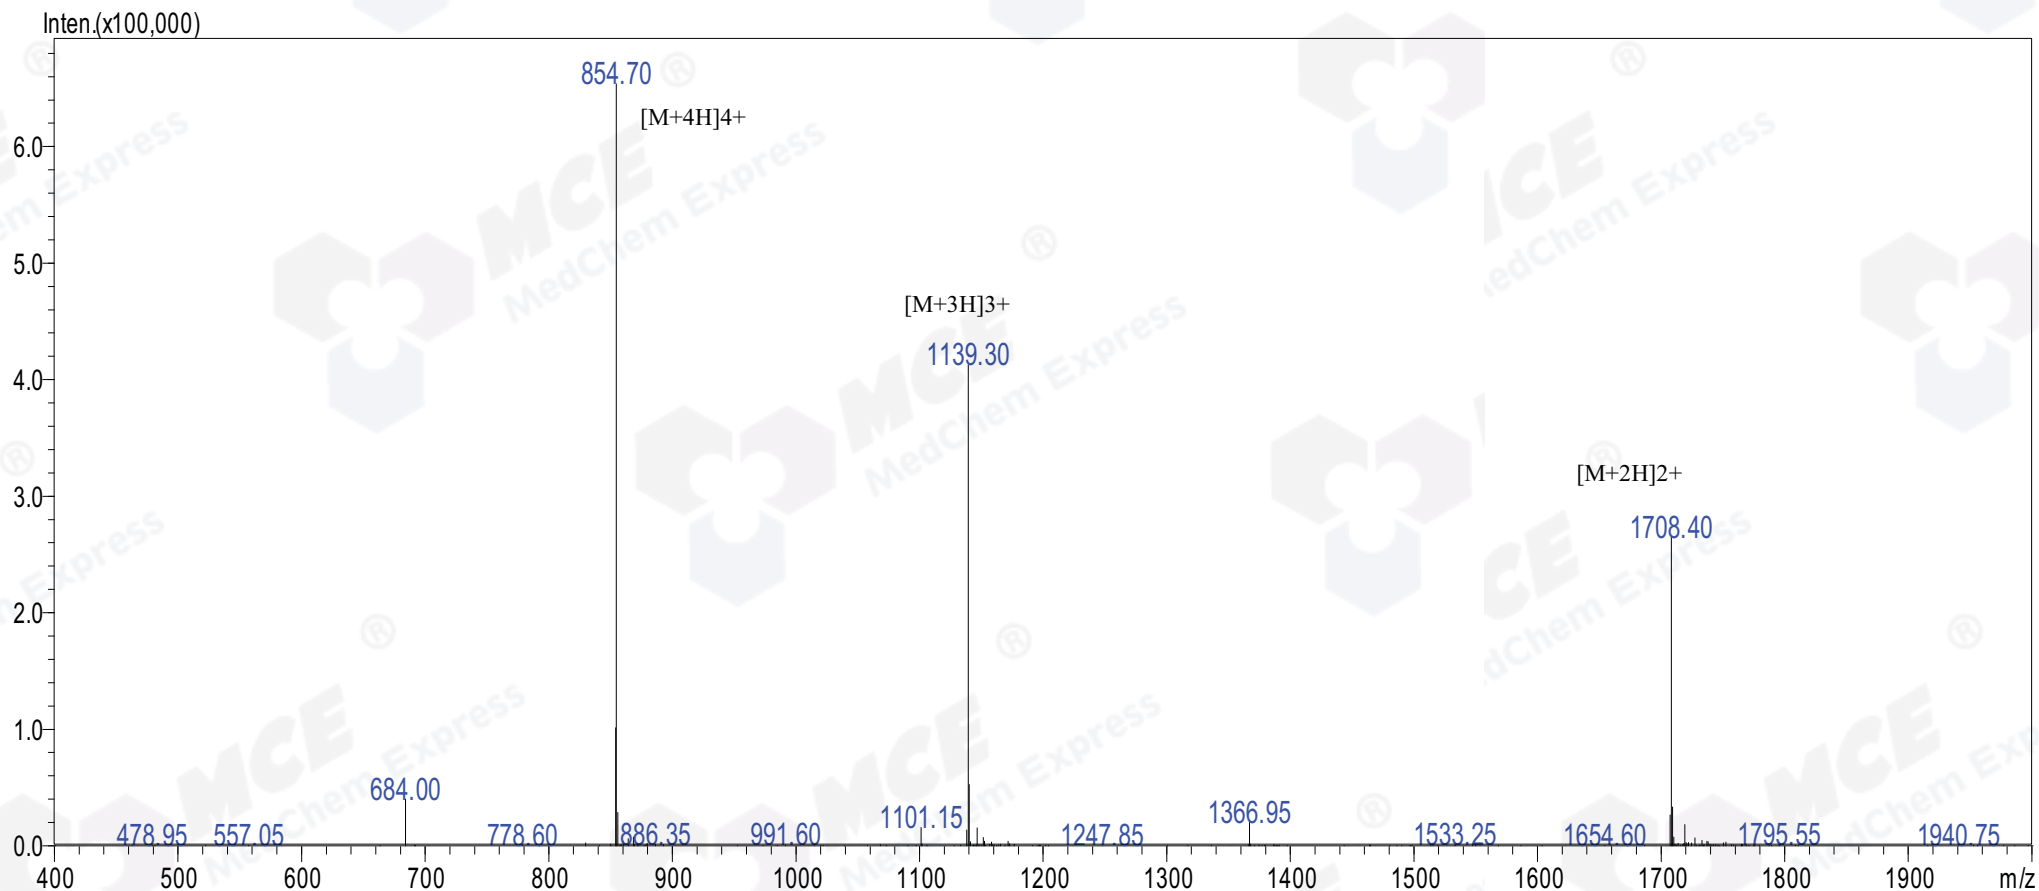

## Sample Description

Analyzed date: 2019-4-3  
Analyst: SHAO  
Sample: 800092  
M.W.: 3414.9  
Catalog No: HY-P1463A Batch#39669

## Instrument

SHIMADZU LCMS-2020  
Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250°C  
Block Temp.: 200°C  
Probe Bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. Conc.: 50%H2O/50%ACN