


Catalog No: HY-P1463A Batch#39669

Data file: E:\DATA\190403\800092 19030017Final.D  
Sample name: 800092 19030017Final  
Description: Mobile phase: Buffer A: 0.1%TFA in H2O  
Buffer B: 0.1%TFA in ACN  
Gradie: 33-43% in 20min, Flow rate: 1.0ml/min  
Column: Unitary C18, 4.6\*150mm, 5um 100A (A-005)  
Instrument: Agilent HPLC 1100

Instrument: QC  
Injection date: 2019/4/3 13:15:57  
Last changed: 2019/4/3 14:33:54

Location: 61  
Injection: 1 of 1  
Injection volume: 5.000  
Acq. operator: QC\_1

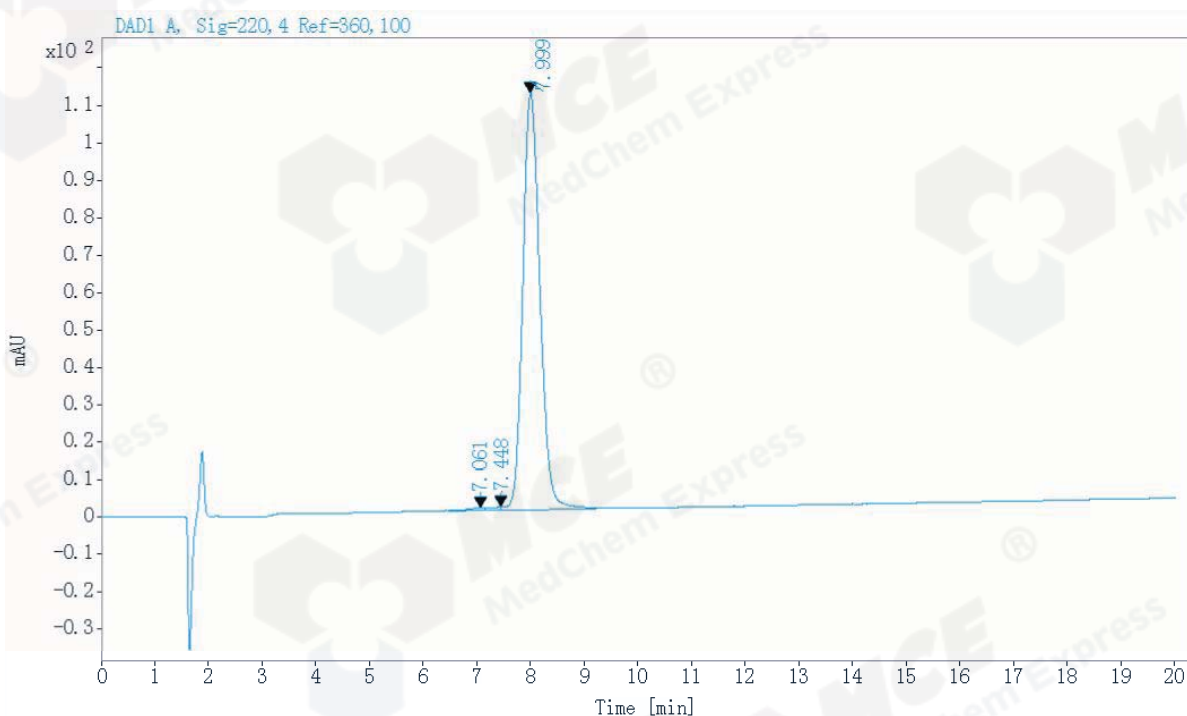

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
7.061	VV	0.3058	16.8139	0.7061	0.6716	
7.448	MF	0.2734	13.4560	0.8203	0.5375	
7.999	FM	0.3697	2473.2925	111.4998	98.7909	
	Sum		2503.5625			