



File ..\DATA\2020\20200608\988\CPK2020-605-SCH11.D Tgt Mass (CHM):
 Injection Date : 8 Jun 20 2:24 pm +0800 Seq. Line : 48
 Sample Name : BIZ2020-605-SCH11 Location : P2-D-06
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200608\988\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200608\988\1-POS-3MIN.M
 Catalog No : HY-P1483A
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

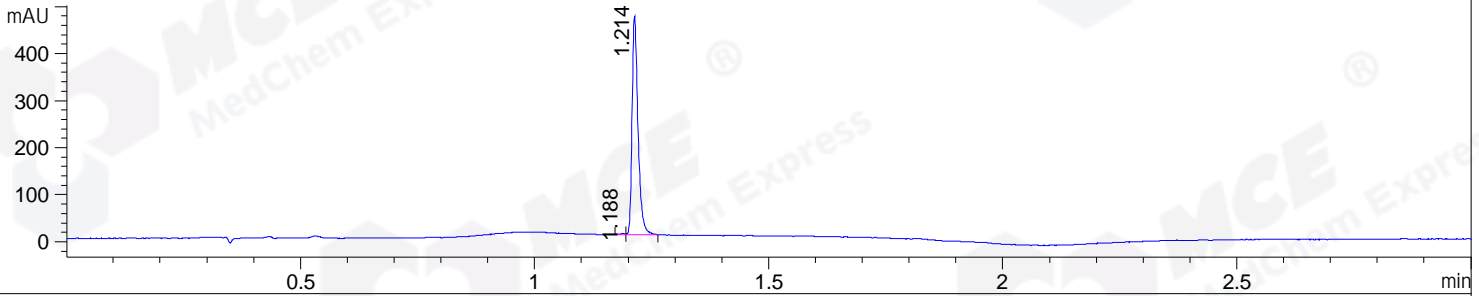

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

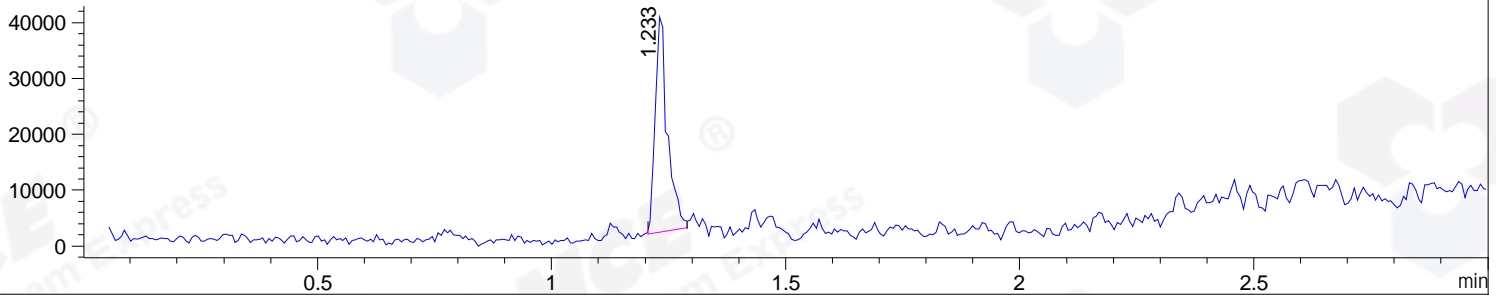

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

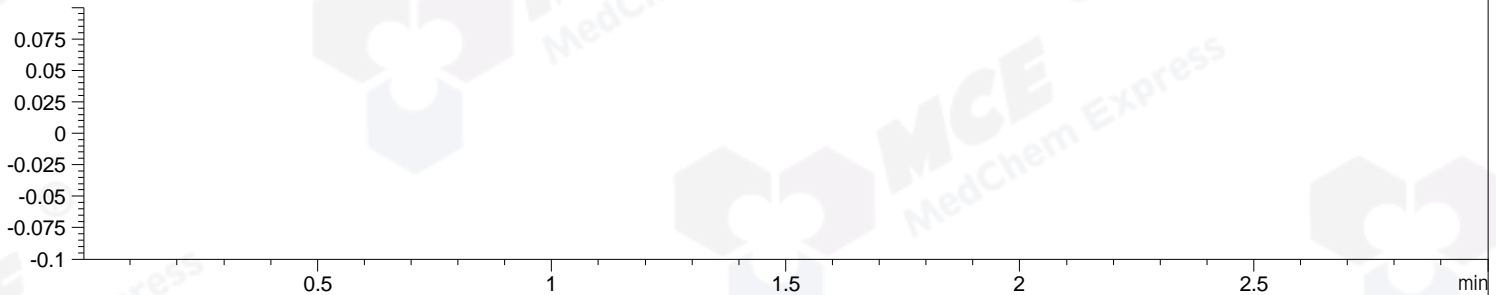

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.19	0.01	1.73	2.12	0.42	ND
1.21	0.01	412.62	464.17	99.58	817

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.03	69901.22	39446.27	100.00	817

Ret. Time: 1.23

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

