

File ..DATA\2019\20190414\561\BIZ2019-412-WYQ20-.D Tgt Mass (CHM):

Injection Date : 14 Apr 19 2:31 pm +0800 Seq. Line : 60

Sample Name : BIZ2019-412-WYQ20 Location : PL-C-09

Acq. Operator : LQ\_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 8 ul

Acq. Method : D:\Chem32\1\data\2019\20190414\561\1-POS-3MIN-1(110-1500).M

Analysis Method : D:\CHEM32\1\DATA\2019\20190414\561\1-POS-3MIN-1(110-1500).M

Catalog No : CS-0089371 Batch#39827

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314

Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

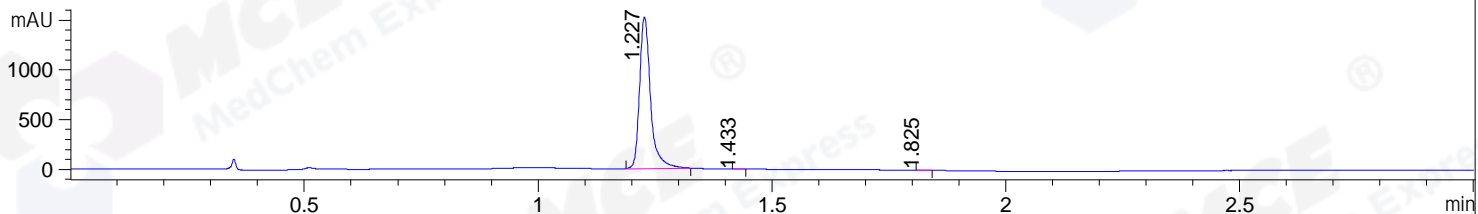


DAD1 C, Sig=254,4 Ref=off

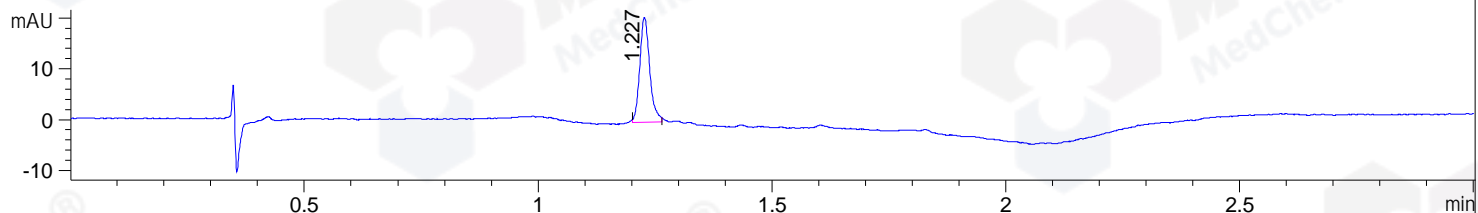

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

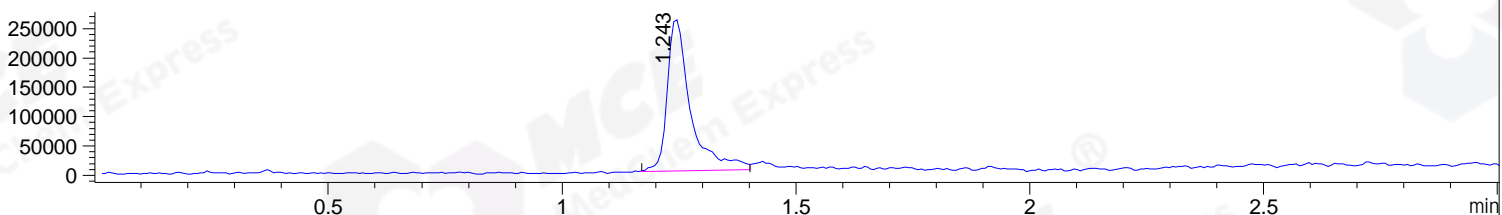

Ion 1077.5, MSD1 1077.5, Target Mass 1076.5 +H Positive, EIC=1077.2:1078.2

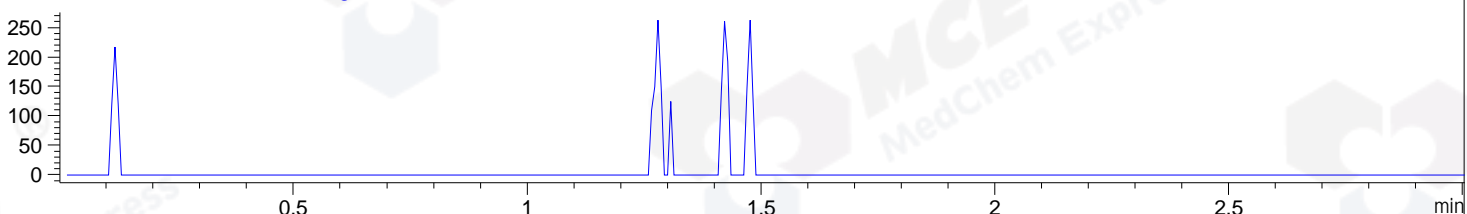

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.02	2513.24	1527.48	99.91	482
1.43	0.02	1.07	0.99	0.04	482
1.83	0.02	1.13	1.00	0.04	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.02	30.59	20.66	100.00	482

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.05	896499.13	260002.73	100.00	482

Ret. Time: 1.24

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

