

File ..\DATA\2019\20190129\551\BIZ2019-129-WYQ11.D Tgt Mass (CHM):

Injection Date : 29 Jan 19 4:50 pm +0800 Seq. Line : 23

Sample Name : BIZ2019-129-WYQ11 Location : P1-E-09

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 5 ul

Acq. Method : D:\Chem32\1\data\2019\20190129\551\1-POS-3MIN-1(500-2000).M

Analysis Method : D:\CHEM32\1\DATA\2019\20190129\551\1-POS-3MIN-1(500-2000).M

Catalog No : HY-P1568A Batch#37226

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)

Gradient: 5% to 95%B within 1.3 min


Flow Rate :1.8ml/min

Column :SunFire C18, 4.6*50mm,3.5um A-RP-314


Oven Temperature : 45C

Postive,MS:500-2000


DAD1 B, Sig=214,4 Ref=off

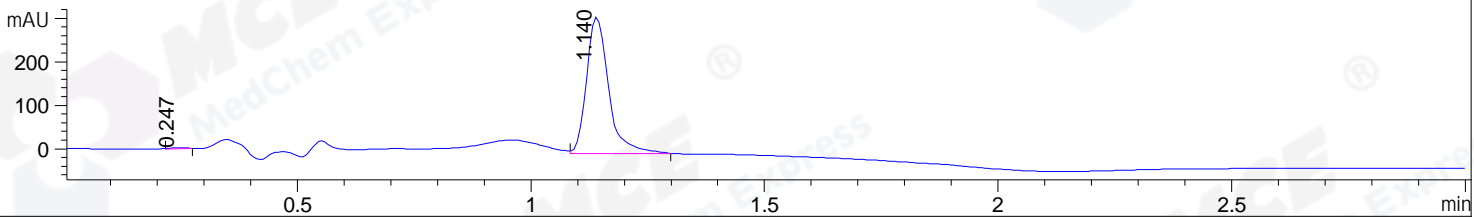


DAD1 C, Sig=254,4 Ref=off

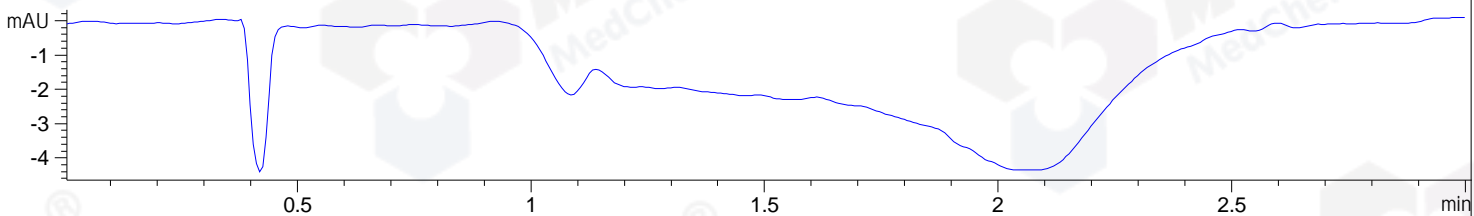

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

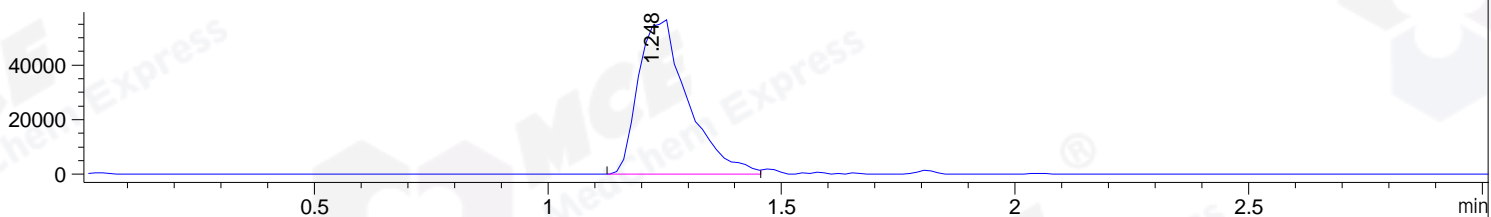

Ion 2273.5, MSD1 2273.5, Target Mass 2272.5 +H Positive, EIC=2273.2:2274.2

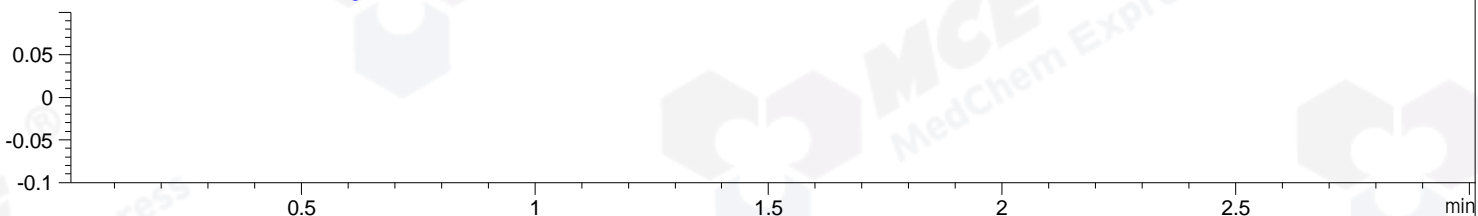

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.25	0.04	6.29	2.69	0.61	ND
1.14	0.05	1029.19	315.25	99.39	759

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
--------	-------	------	--------	-------	--------

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.11	417638.09	58153.96	100.00	759

Ret. Time: 1.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

