

File ..DATA\2019\20190118\546\BIZ2019-118-WYQ7-1.D Tgt Mass (CHM):

Injection Date : 18 Jan 19 4:20 pm +0800 Seq. Line : 16

Sample Name : BIZ2019-118-WYQ7 Location : P1-D-08

Acq. Operator : LQ\_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 2.5 ul

Acq. Method : D:\Chem32\1\data\2019\20190118\546\1-POS-3MIN-1(110-1500).M

Analysis Method : D:\CHEM32\1\DATA\2019\20190118\546\1-POS-3MIN-1(110-1500).M

Catalog No : HY-P1574A Batch#36949

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314

Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

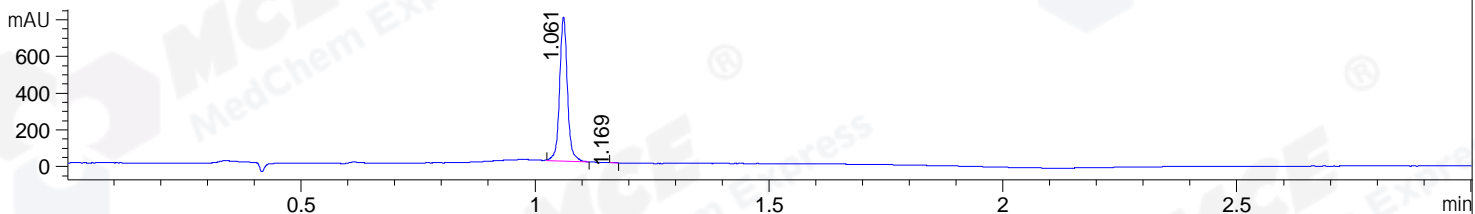


DAD1 C, Sig=254,4 Ref=off

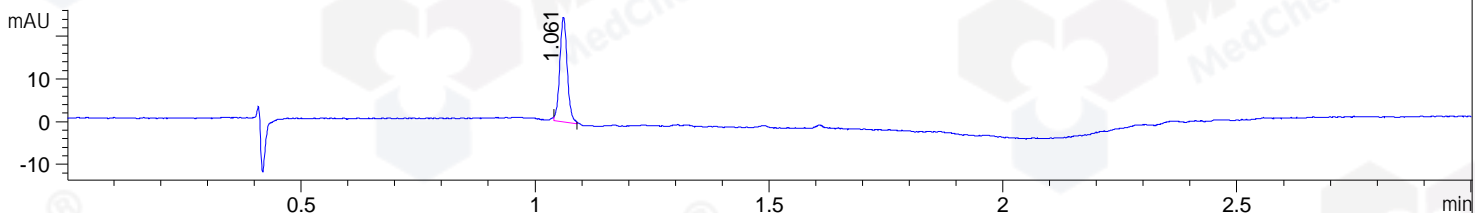

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

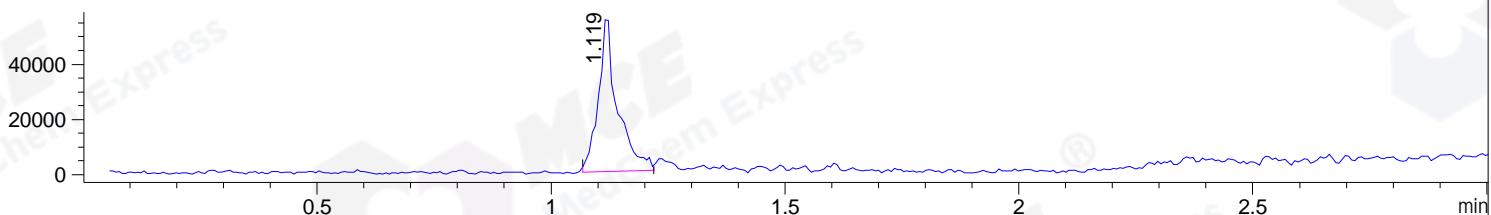

Ion 1051.2, MSD1 1051.2, Target Mass 1050.2 +H Positive, EIC=1050.9:1051.9

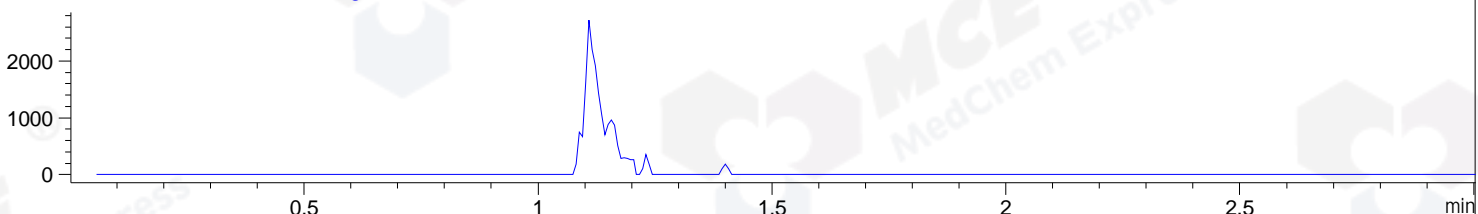

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.06	0.02	911.96	784.94	99.87	526
1.17	0.01	1.21	1.66	0.13	526

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.06	0.02	27.23	24.57	100.00	526

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.04	158011.38	57325.64	100.00	526

Ret. Time: 1.12

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

