


# MASS SPECTROMETRY REPORT

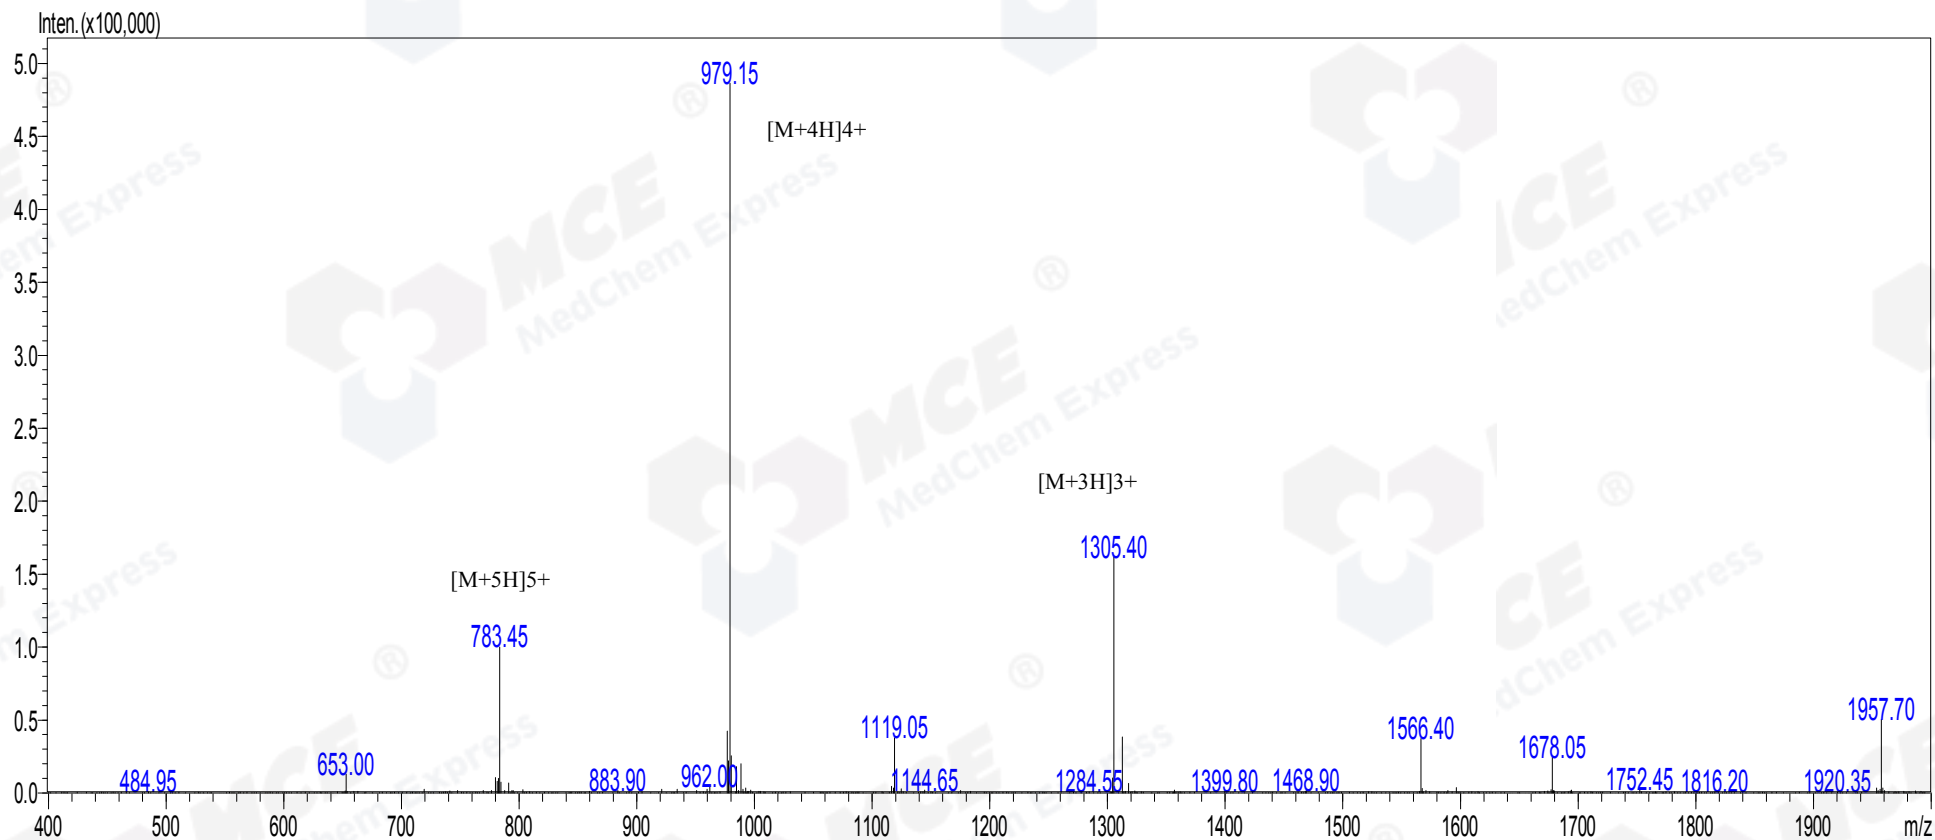

## Sample Description

Analyzed date: 2020-11-6  
Analyst: SHAO  
Sample: 602977  
M.W.: 3912.4  
Catalog No: HY-P1871A

## Instrument

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250°C  
Block Temp.: 200°C

## SHIMADZU LCMS-2020

Probe Bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. Conc.: 50%H2O/50%ACN