
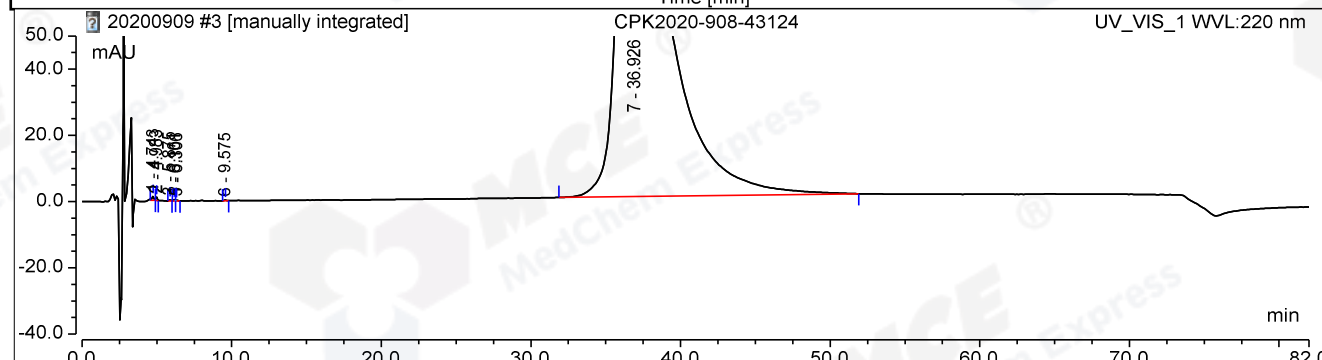


Chromatogram and Results

Injection Details			
Injection Name:	CPK2020-908-43124	Injection Volume:	100.00
Vial Number:	RC7	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	220
Calibration Level:		Users:	jlw
Instrument Method:	HY-P1923-H01P01(RP-HPLC)	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	09/Sep/20 12:20	Run Time (min):	82.00
Comment:	HY-P1923-20190710 A-RP-420		
chrom://hy261/Themo/Instrument Data/202009/20200909.seq/418.smp/UV_VIS_1.channel/UV_VIS_1.chm			

Chromatogram

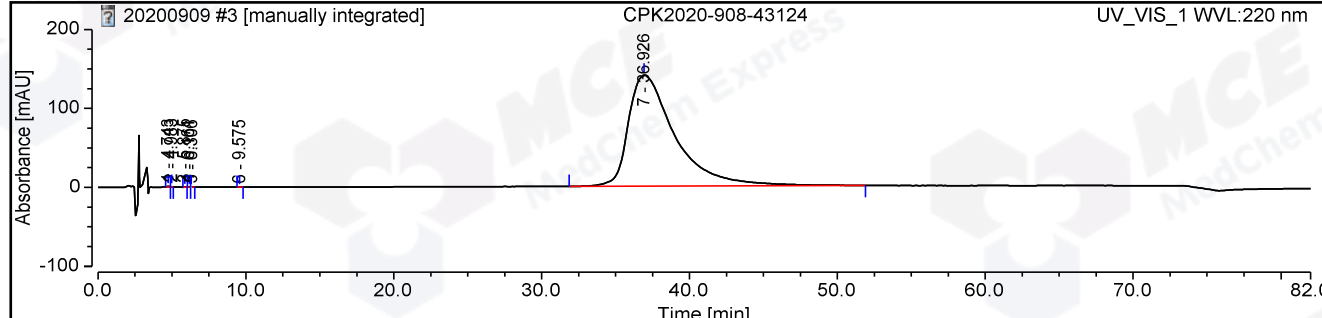

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	S/N	Rel.Area %
1		4.743	0.185	1.223	0.94	0.1	0.04
2		4.983	0.090	1.033	1.09	0.1	0.02
3		5.875	0.054	0.483	1.01	0.0	0.01
4		6.161	0.043	0.369	n.a.	0.0	0.01
5		6.306	0.028	0.164	n.a.	0.0	0.01
6		9.575	0.039	0.254	1.19	0.0	0.01
7		36.926	513.029	140.841	1.89	9.1	99.91
Total:			513.469	144.367	6.12	9.30	