


MASS SPECTROMETRY REPORT

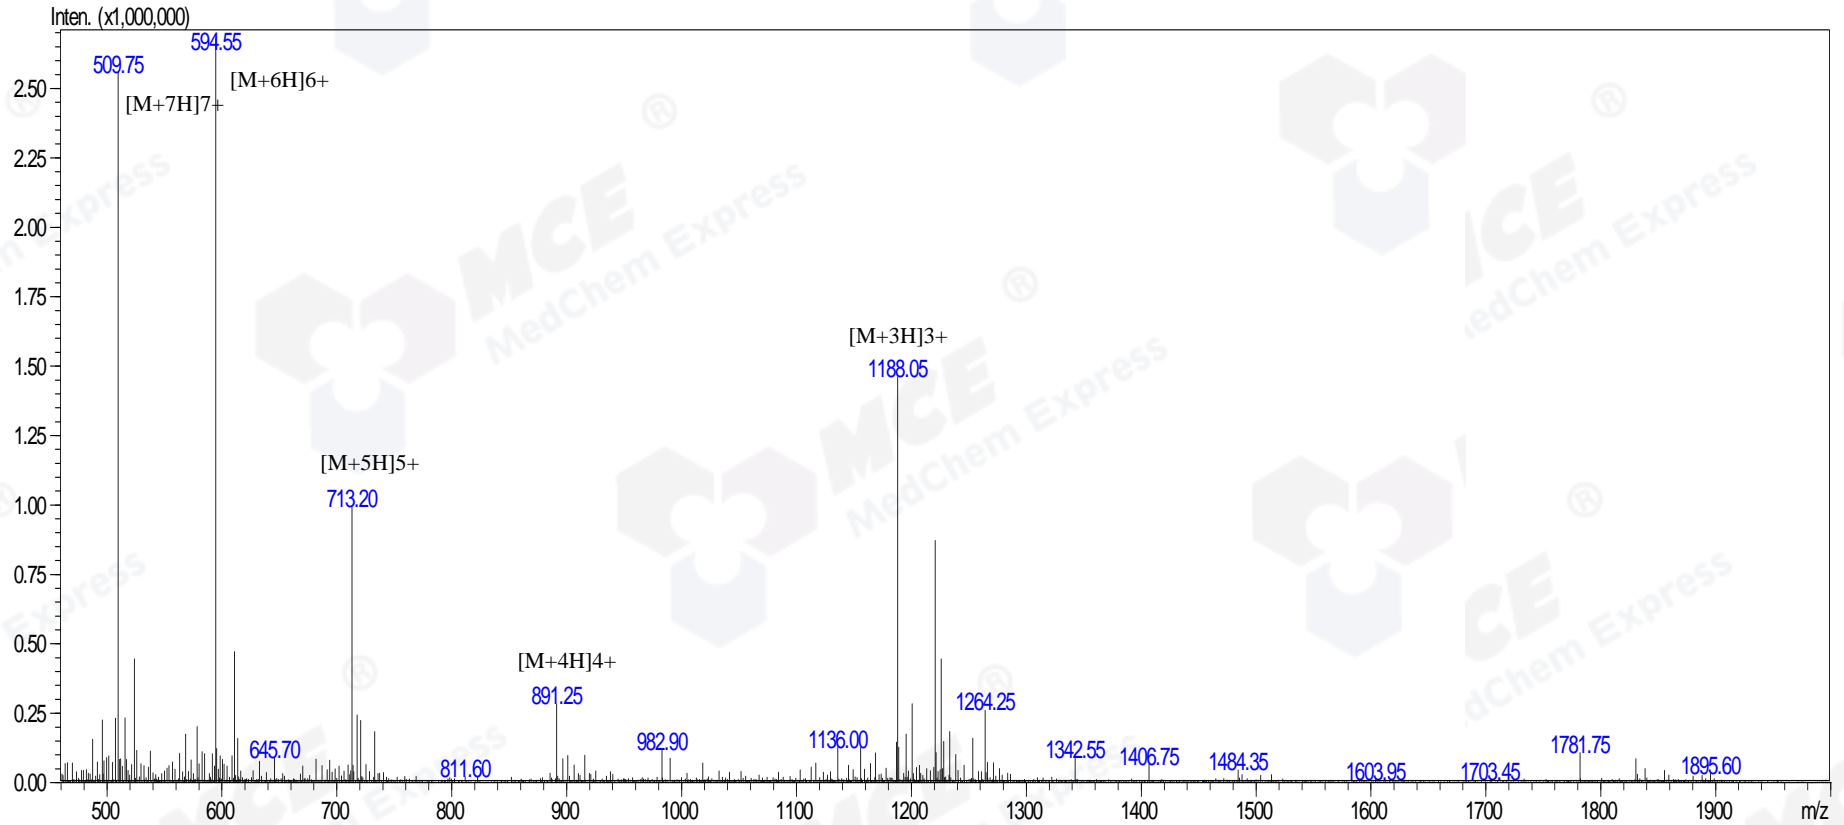

Sample Description

Analyzed date: 2020/6/28

Analyst: Shen

Sample: 1220751-16-5 GI-31

M.W.: 3561.07

Catalog No: HY-P2262A

Instrument

Probe:

Nebulizer Gas Flow: 1.5L/min

CDL:

CDL Temp.: 250 °C

Block Temp.: 400 °C

SHIMADZU LCMS-2020

ESI

1.5L/min

-20.0v

250 °C

400 °C

Probe Bias:

Detector:

T. Flow:

B. Conc.:

+4.5kv

1.2kv

0.2ml/min

50%H2O/50%ACN