


# .MASS SPECTROMETRY REPORT

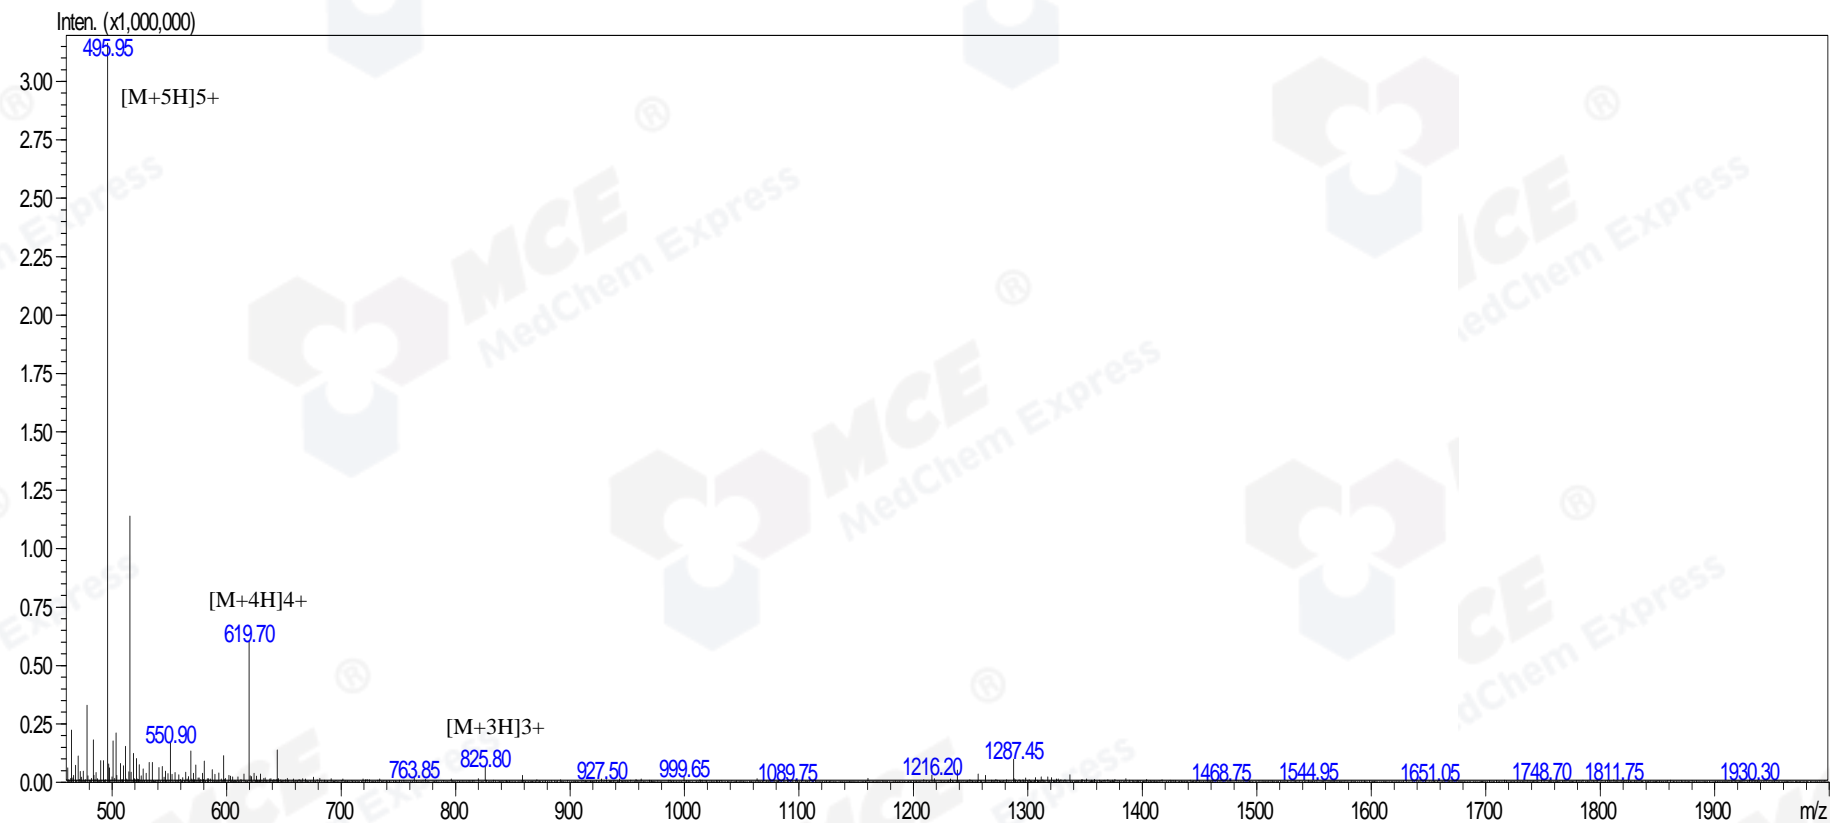

## Sample Description

Analyzed date: 2020/6/23

Analyst: Shen

Sample: 847829-41-8 YA-20

M.W.: 2474.88

Catalog No: HY-P2307

## Instrument

Probe:

Nebulizer Gas Flow: 1.5L/min

CDL:

CDL Temp.:

Block Temp.:

SHIMADZU LCMS-2020

ESI

1.5L/min

-20.0v

250 °C

400 °C

Probe Bias:

Detector:

T. Flow:

B. Conc.:

+4.5kv

1.2kv

0.2ml/min

50%H2O/50%ACN