


SEC-HPLC


Analysis Report

<Chromatogram>

mV

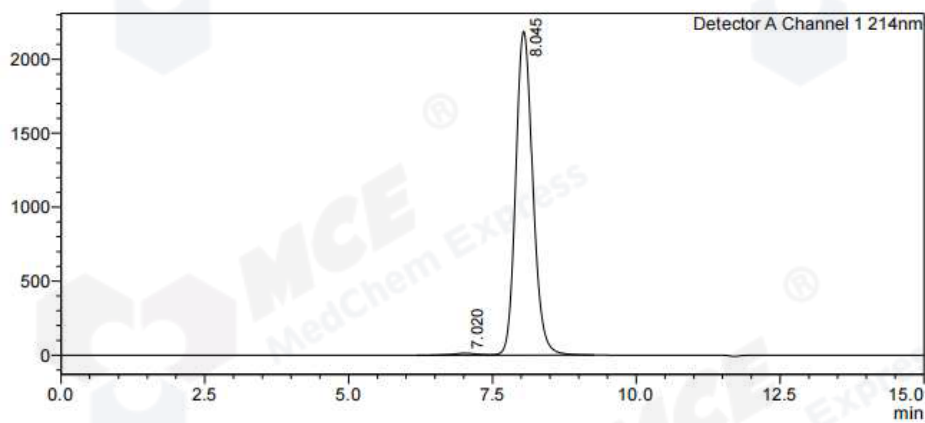

mV

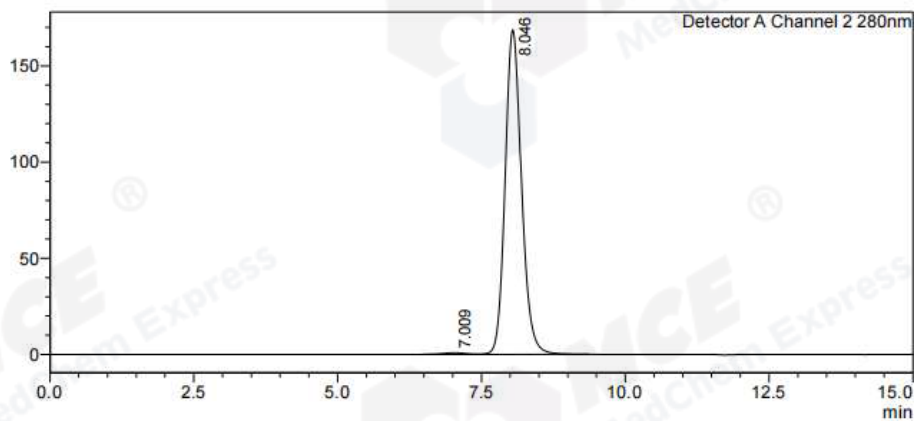

<Peak Table>

Detector A Channel 1 214nm

Peak#	Ret. Time	Area	Height	Conc.
1	7.020	401286	13140	0.879
2	8.045	45251086	2186492	99.121
Total		45652373	2199631	

Detector A Channel 2 280nm

Peak#	Ret. Time	Area	Height	Conc.
1	7.009	28871	918	0.855
2	8.046	3347649	168554	99.145
Total		3376520	169473	

The purity of B7400 is more than 95% verified by SEC-HPLC.