
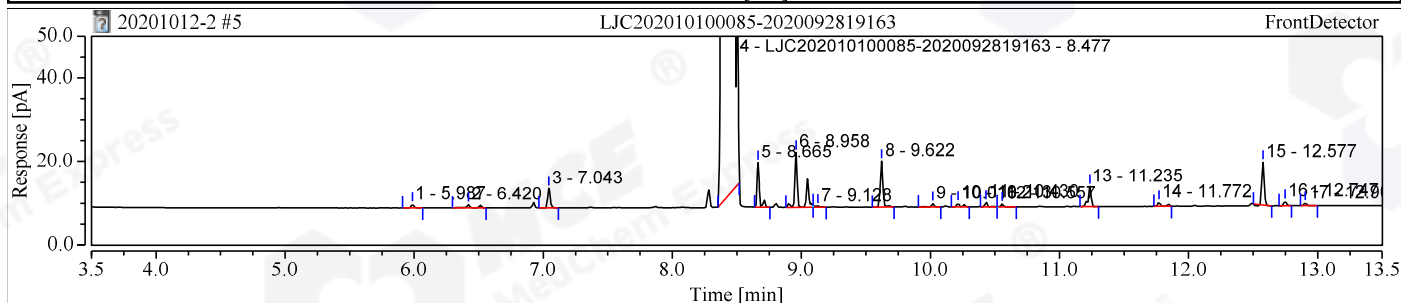


## Chromatogram and Results

Catalog No:	HY-W007346	Channel:	FrontDetector
Vial Number:	5	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Calibration Level:	AHC008	Injection Time:	12/10/2020 18:15
Instrument Method:	GC-FQ	InstMeth.creation_time:	11/05/2020 11:09
Processing Method:	PM-LJC202010100085-2020092819163	Last update_time:	13/10/2020 13:26
seq.creation_operator:	Ayuxp	Data Operator:	mlill
Comment:	GC-202004	Print Operator:	Ayuxp

chrom://ahyy-cm7/CM7DATA/Leyan/AHC008/Sequence/20201012-2.seq/129.smp/FrontDetector.channel/FrontDetector.chm

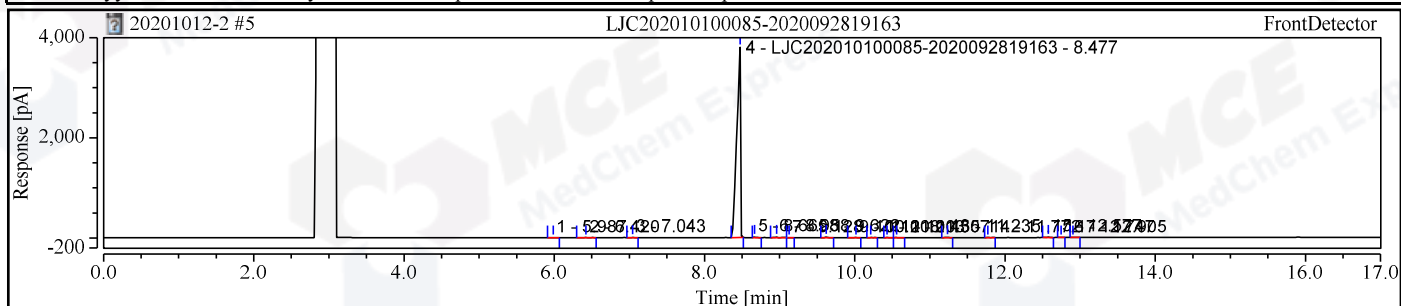

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	5.987	0.020	0.924	540160	12.95	1.15	0.01	
2	6.420	0.040	0.818	558932	18.41	0.63	0.02	
3	7.043	0.099	4.651	712160	22.79	1.18	0.04	
4	8.477	220.553	3792.791	134694	3.07	0.56	99.28	10100085-2020092
5	8.665	0.237	10.659	1310104	9.55	1.01	0.11	
6	8.958	0.430	13.138	1324845	3.67	1.02	0.19	
7	9.128	0.016	0.298	353513	10.13	n.a.	0.01	
8	9.622	0.258	10.977	1145400	11.54	0.95	0.12	
9	10.018	0.021	0.837	1492040	6.04	1.00	0.01	
10	10.213	0.028	0.885	1657181	6.99	0.94	0.01	
11	10.430	0.022	1.097	1896208	4.05	1.02	0.01	
12	10.557	0.017	0.744	1717906	20.82	0.97	0.01	
13	11.235	0.123	4.826	1860114	16.25	0.74	0.06	
14	11.772	0.031	1.008	2021173	23.70	1.01	0.01	
15	12.577	0.205	10.213	2086695	4.54	1.00	0.09	
16	12.747	0.027	1.026	1614535	3.90	1.17	0.01	
17	12.905	0.017	0.610	1572339	n.a.	1.01	0.01	
<b>Total:</b>		<b>222.143</b>	<b>3855.502</b>	<b>21997999.000</b>	<b>178.38</b>			