


Software Version : 6.3.1.0504
Sample Name : LJ1707110014 1026154
Instrument Name : CLARUS 600
Rack/Vial : 0/62
Sample Amount : 1.000000
Cycle : 1

Date : 2017-7-13 16:18:18
Data Acquisition Time : 2017-7-13 13:33:11
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File :
Sequence File : D:\sequence\170713.seq

Catalog No: HY-W007692 Batch# 45749

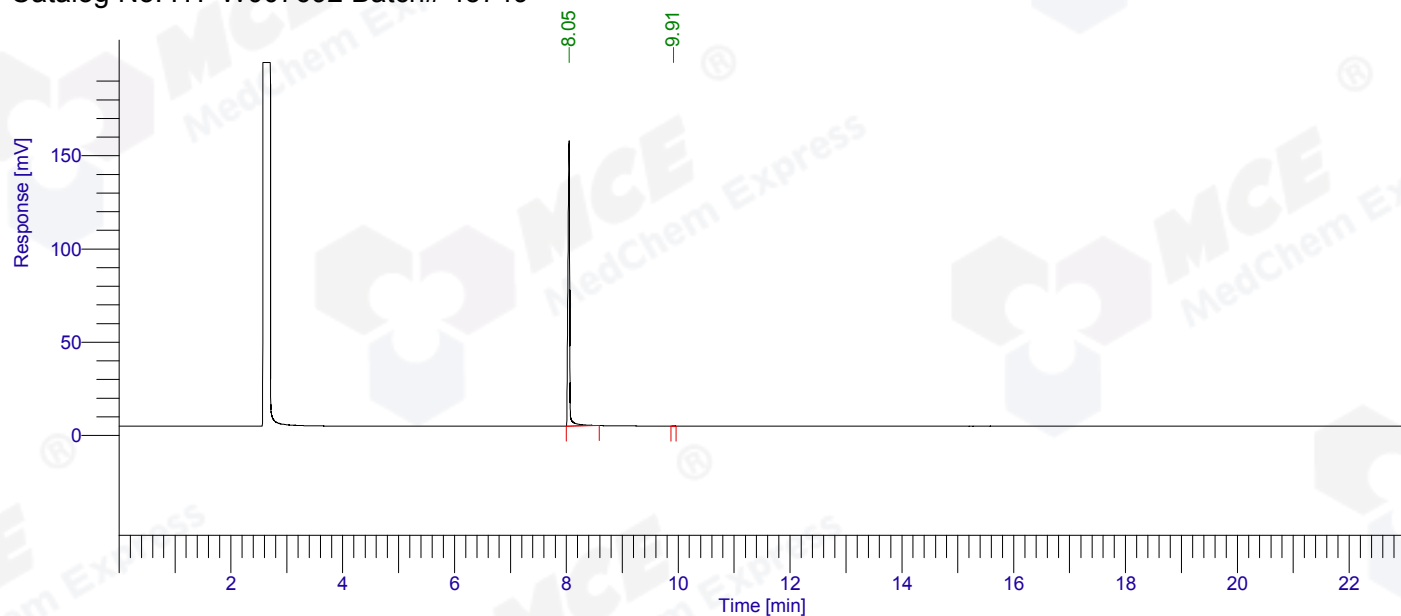

Area Percent Report

| Peak # | Component Name | Time [min] | Area [UV*sec] | Area Percent [%] |
|--------|----------------|------------|---------------|------------------|
| 1 | | 8.048 | 330832.49 | 99.9545 |
| 2 | | 9.915 | 150.68 | 0.0455 |
| | | | 330983.17 | 100.0000 |

Missing Component Report
Component Expected Retention (Calibration File)

All components were found